EN

Step-by-Step Guide:

Chlamydia Antigen Rapid Test Kit

The Chlamydia Rapid Test Device detects Chlamydia antigen in clinical specimens using lateral flow immunoassay technology, providing rapid qualitative results within 15 minutes. The test contains antibodies specific to Chlamydia antigen coated on the test region of the membrane. During testing, the extracted antigen solution reacts with antibody-coated particles.

If Chlamydia antigen is present, a red line forms in the test region, indicating a positive result. The absence of this line suggests a negative result. A red control line always appears to confirm proper specimen volume and membrane function. Accuracy is 98.2%.

Precautions & Specimen Collection:
For professional use only. Wear protective gear, handle safely, and follow disposal guidelines. Use whole blood, serum, or plasma. Store at 2-8°C (3 days) or below -20°C (long-term) and bring to room temperature before testing.

Storage:
Store in a sealed pouch at 2-30°C, do not freeze, and use before the expiration date.

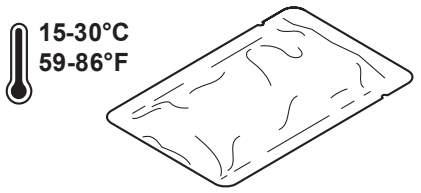

1 Preparation

Before starting the test, open the test kit package and take out all components.

Kit Contents:
- Test device (individually packed)
- Extraction tube with buffer A
- Buffer B
- Sterile swabs
- Step-by-Step Guide

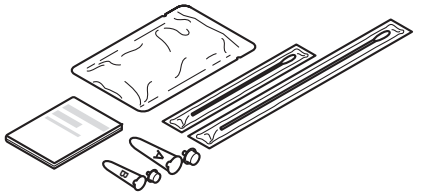

Open the pouch and place the test device on a flat surface

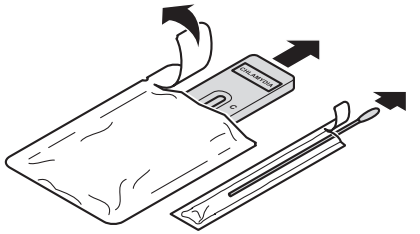

2 Sample Collection

Use the sterile swabs from the kit. **Female**: Insert the long swab into the endocervical canal until most of the tip is hidden. Rotate it 360° in one direction, wait 15 seconds, then remove it. **Male**: Insert the swab into the urethra about 2-4 cm, 360° in one direction, wait 10 seconds, then remove it.

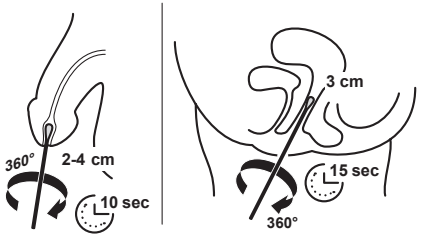

Insert the cervical or urethral swab into the extraction tube with buffer A. Roll it 15 times while pressing against the tube A. Wait for 2 minutes.

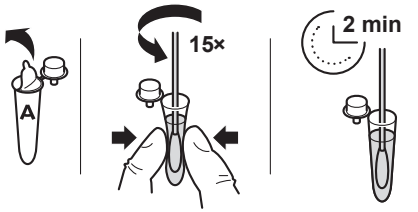

Add 9 drops of Buffer B solution into the extraction tube with buffer A. Roll it 15 times while pressing against the tube A.

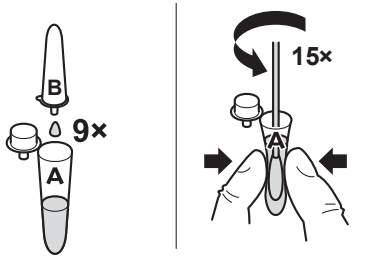

Wait for 1 minute and squeeze out excess liquid as you remove the swab.

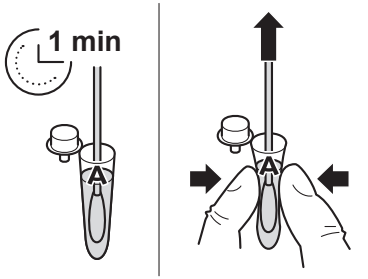

3 Test Procedure

Add 3 drops of the specimen to the sample well.

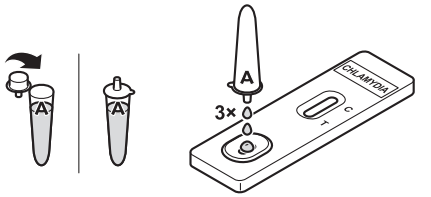

Wait 10 minutes and read the results. Do not interpret after 30 minutes.

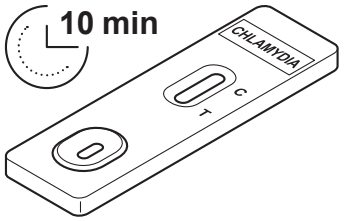

4 Result Interpretation

Positive: If two lines appear at C and T, the result is Chlamydia Positive. In all positive cases, consult a healthcare professional for further evaluation and guidance.



Negative: Only one line appears at C. No detectable Chlamydia antibodies. If symptoms persist, repeat the test after the incubation period or consult a healthcare professional for further evaluation.



Note: The intensity of the red color in the test line region (T) may vary depending on the concentration of Chlamydia antigen presents in the specimen. Therefore, any shade of red in the test region (T) should be considered positive.

Invalid: If no line appears at C, the test did not work correctly and is invalid. Use a new test device and follow the instructions carefully.



Remedium Biotech Solutions, incorporated in Singapore, manufactures rapid test kits for STDrapidtestkits.com, offering accurate, convenient, and discreet at-home STD testing. With over 20 years of experience, we produce ISO 13485, GMP, and CE-certified test kits that deliver reliable results within minutes.

Our test kits are available worldwide, with local distributors ensuring fast and discreet delivery. For accurate results, follow all instructions carefully. Testing too early may result in false negatives, as antibodies may not yet be detectable. If symptoms persist despite a negative result, consult a healthcare professional.

This test is for preliminary screening only and should not replace a professional medical diagnosis. For confirmation, seek testing from a qualified healthcare provider. The manufacturer and distributor are not responsible for any misuse or reliance on test results.

helpdesk@stdrapidtestkits.com
stdrapidtestkits.com